




# Therapeutic setting of the hammock Moki (MOK16-33)

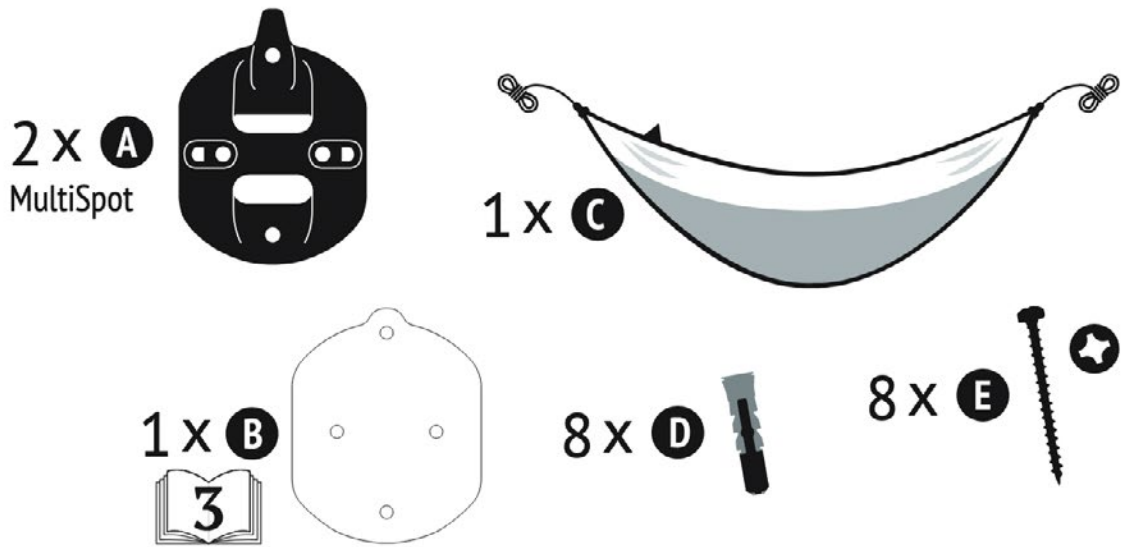


1

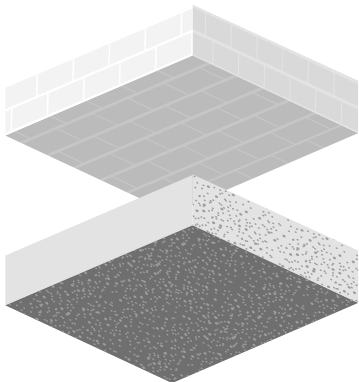






Min. 8,5 cm  
Min. 3.3 Inches





Min. 4 cm  
Min. 1.6 Inches

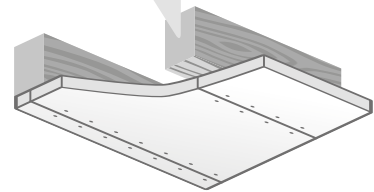


2

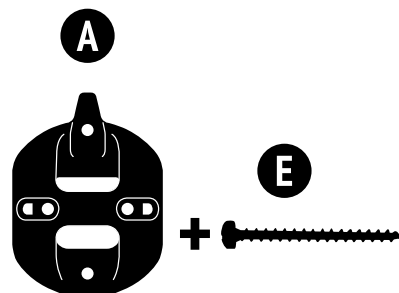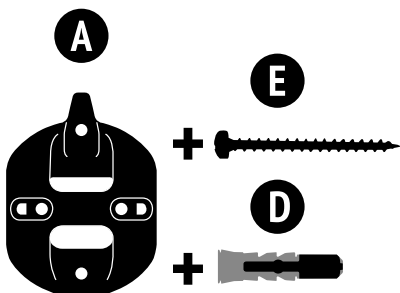


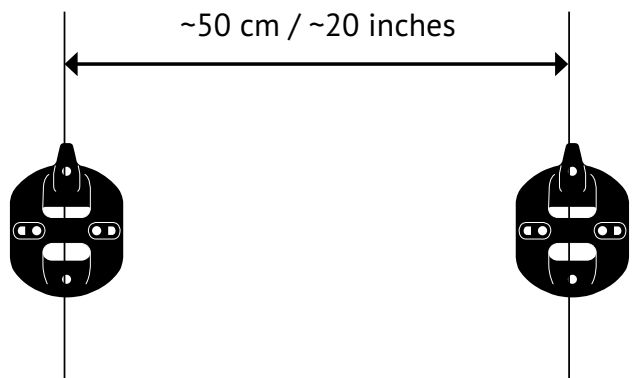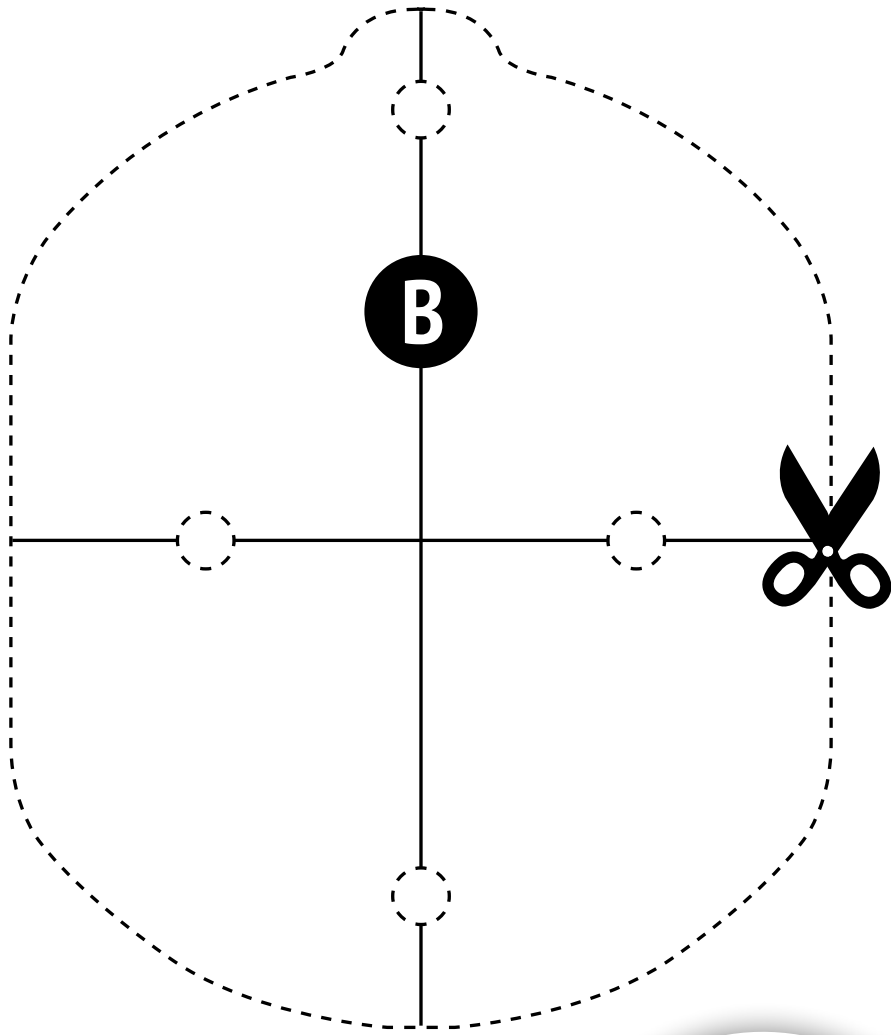


# 2a

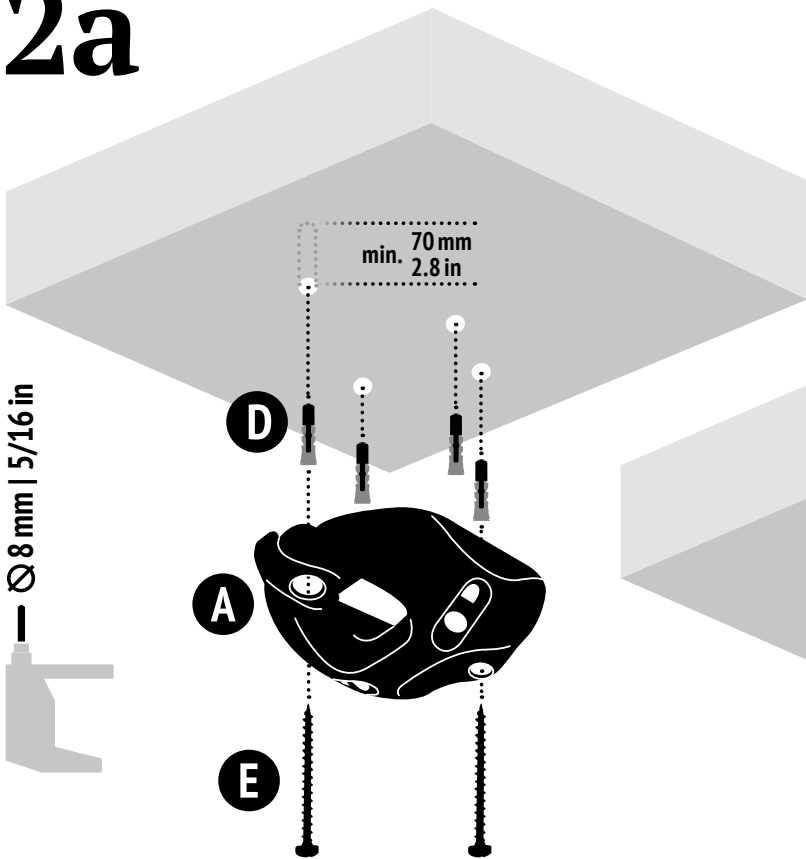


Ø 8 mm | 5/16 in

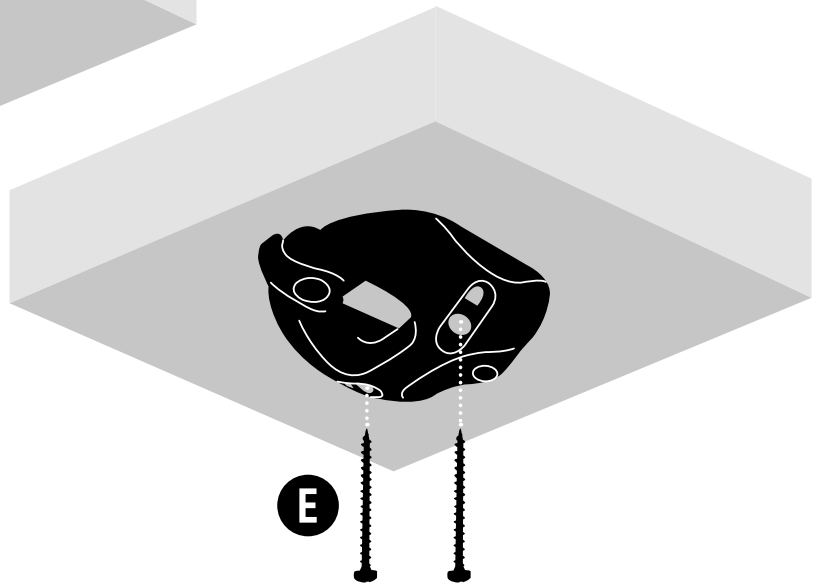

2b


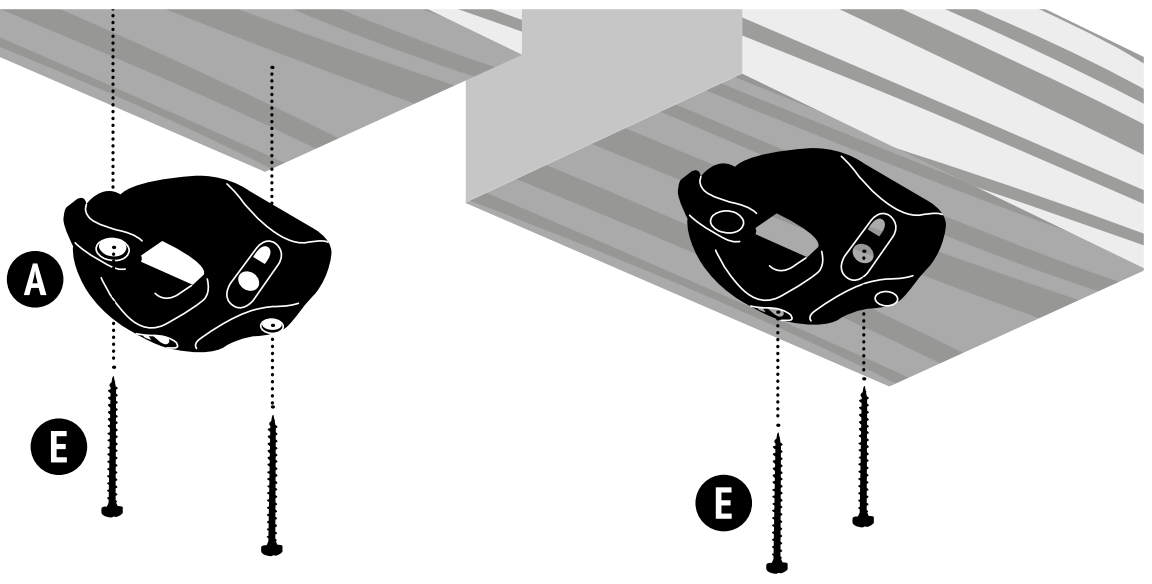


2c

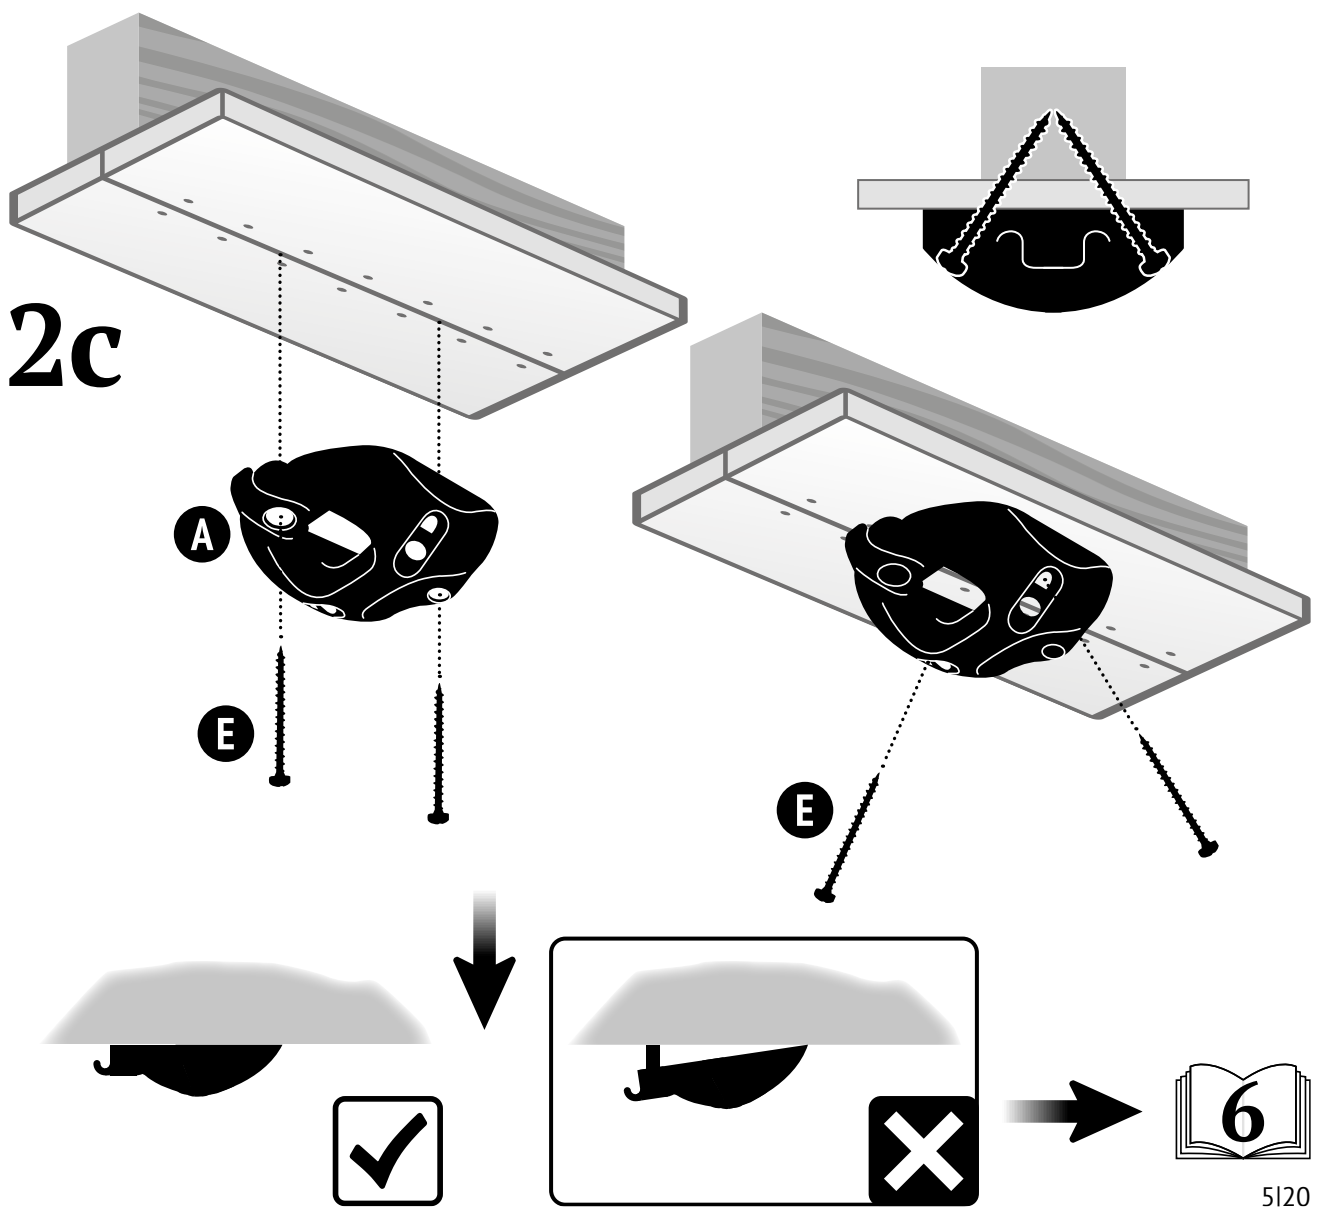



5120

3

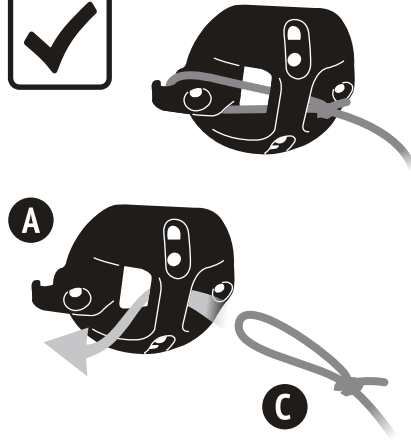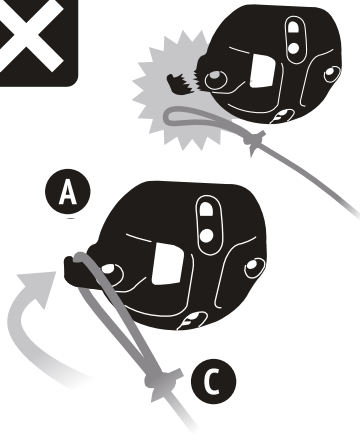



Height  
adjustment

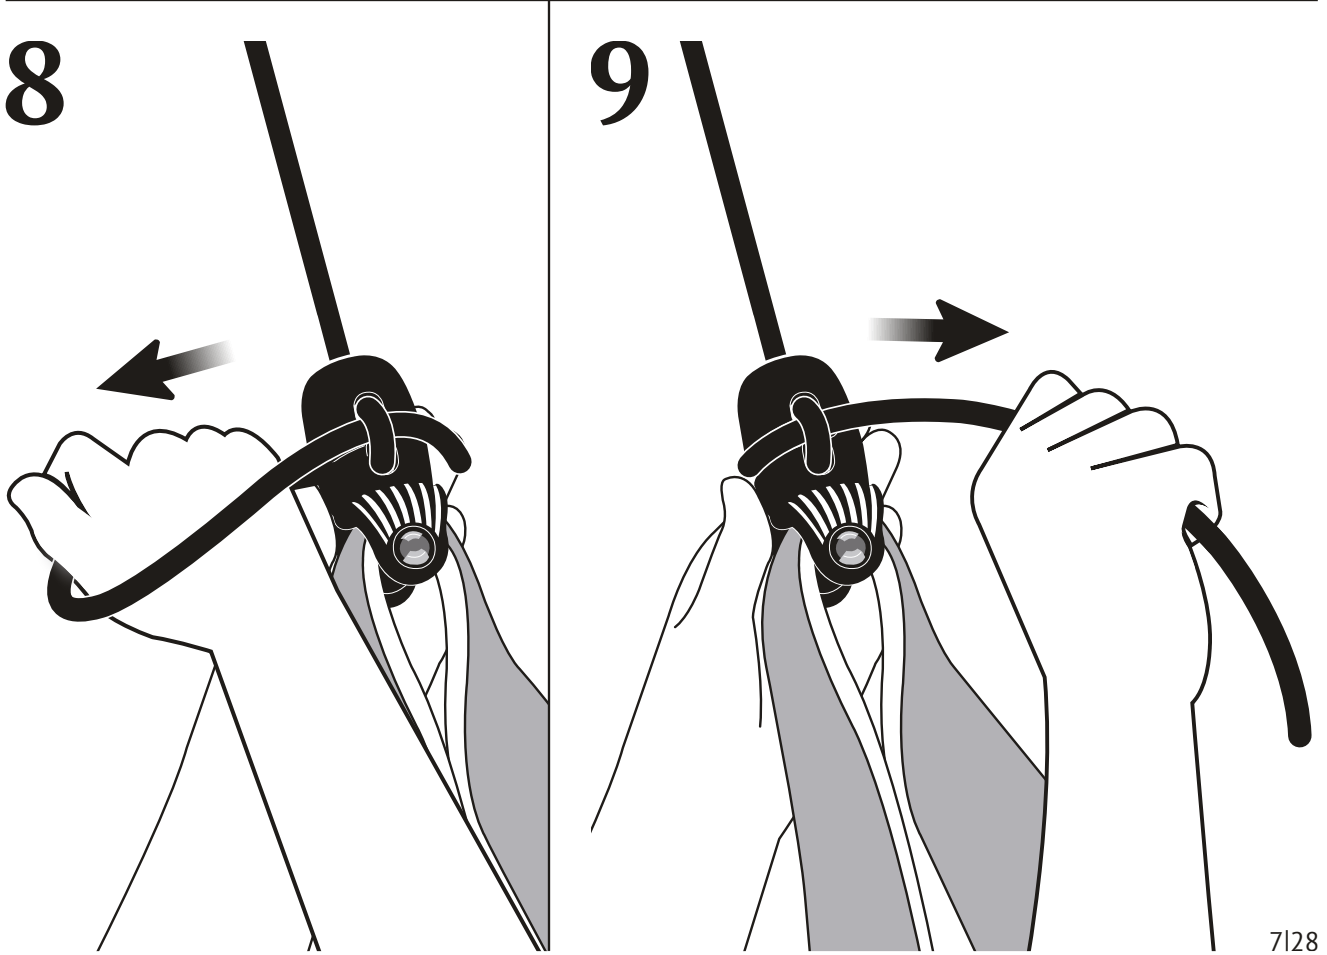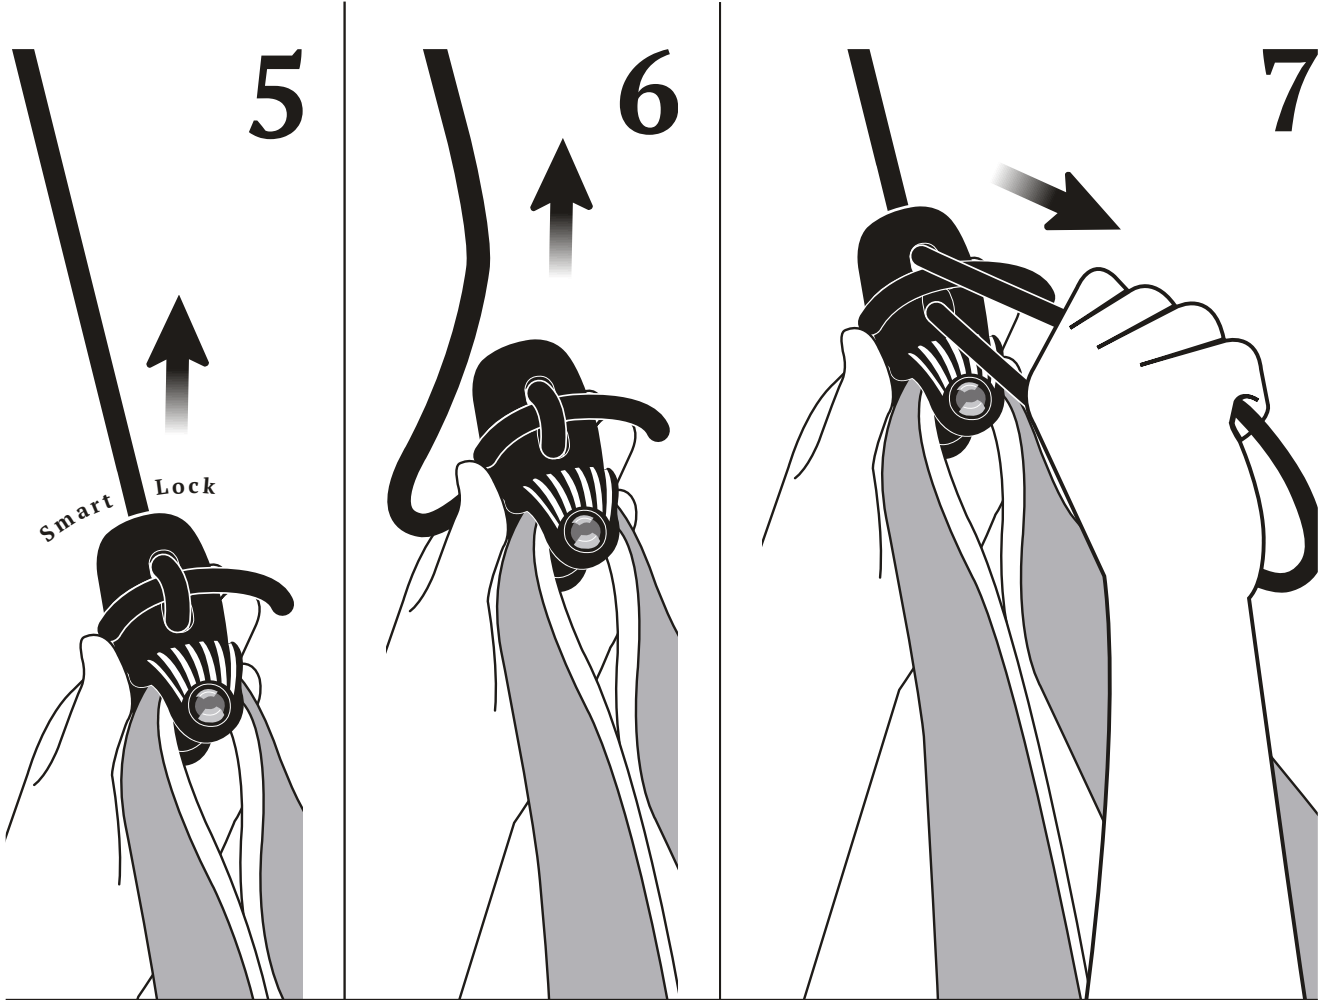

For Security and Care instructions,  
see the instruction manual of MOK16:  
[https://media.lasiesta.com/mediafiles/InstructionSheets/MOK\\_Manual\\_22-08-B.pdf](https://media.lasiesta.com/mediafiles/InstructionSheets/MOK_Manual_22-08-B.pdf)

